

SurgiTel Face Shield Usage Instructions

(Patent-Pending Design)

- Push out pre-scored vertical slot if you wish to have your light protrude from shield. If you wish to try your light behind shield, DO NOT punch out vertical slot.
- Face shield sent with protective film to protect from scratching. Remove from both sides before using.
- Usage Duration: Per CDC recommendations, it is okay to use products which are in limited supply as long as they are safe to use. When the shield clarity is reduced, it must be replaced. Customers are to always follow the current CDC recommendations. Customers should check www.cds.gov regularly for updates.
- Disinfection: Customers may use any materials they feel is required to meet their disinfection requirements. Optim 1 is recommended.
- If you require additional space behind your face shield for larger loupes, or to use your light without punching out vertical slot: see instructions at the bottom of this page
- Attaching a Universal Clip Adaptor: See instructions on reverse side

See images below for examples of different loupe and light usage.

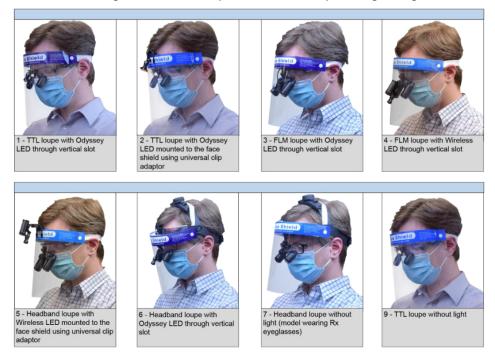

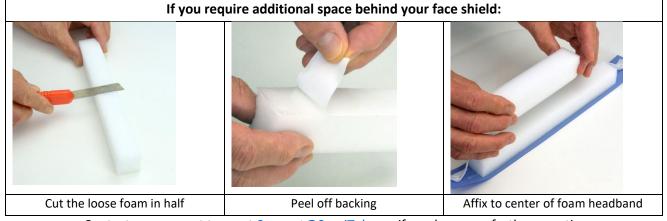


Contact our support team at Support@SurgiTel.com if you have any further questions.

Thank you for your purchase!

Doc. No.: 26820A Page 1 of 2

Instructions for attaching a Universal Clip Adaptor (Optional)

If you are using a Universal Clip Adaptor you will need: your adaptor, your face shield, a pen or marker, and a thin screwdriver or similar instrument.

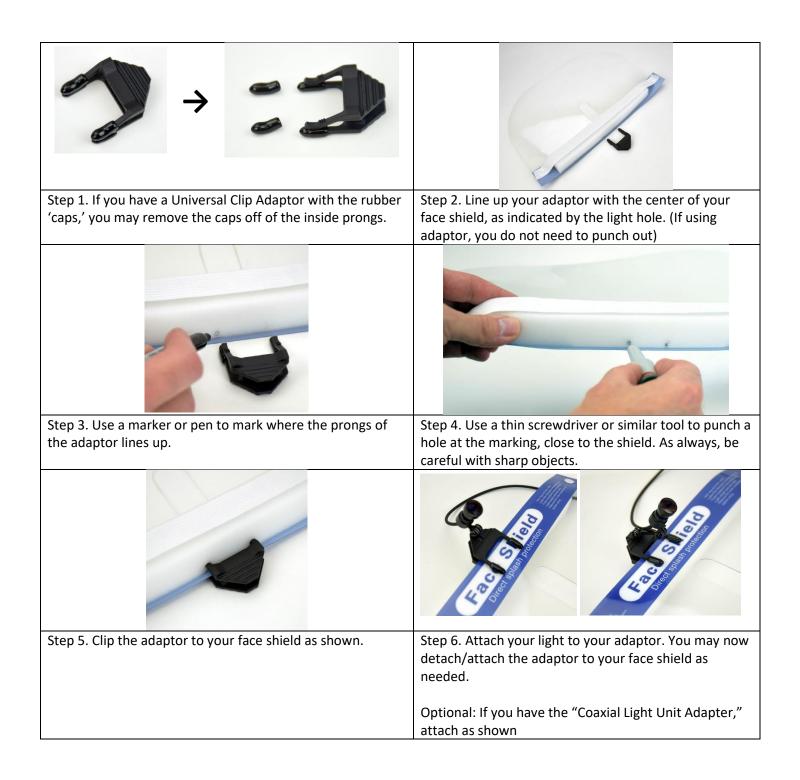

Doc. No.: 26820A Page 2 of 2